

What Does It Measure?

The Tewameter® TM Hex (successor of the worldwide acknowledged Tewameter® TM 300) assesses the **Transepidermal Water Loss (TEWL)**, indispensable parameter for the evaluation of the water barrier function of the skin, with **utmost accuracy and reproducibility**.

The Measuring Principle


Water is constantly **evaporating** from the skin which is part of the important body's metabolism. The **amount of water (TEWL)** is expressed in $g/h/m^2$. **30 sensors** inside the hollow cylinder of the probe „see“ the **relative humidity and temperature** like a camera. The high amount of data allows the user not only to measure **inside the probe** with high accuracy, but can show results also for the areas right outside the probe, namely **skin surface and ambience** above the probe. Thus, **new, exciting parameters** (local skin energy balance and others) may give interesting insights in several research fields.

Fields of Application

- Indispensable in formulation, **efficacy testing and claim support** for cosmetics and pharmaceuticals, regarding improvement of the skin barrier function.
- **Safety tests** for products as even slight deficiencies in the skin barrier can be detected.
- Dermatological **basic research**.
- **Sweat studies** (anti-perspirant efficacy testing).
- **Patch Tests**
- Educative measurement in **occupational health** to alert people for the necessity of using skin protection products.
- **Veterinary medicine** and zoology.
- Also for the textile, food, packaging and paper/tissue **industry**, the measurement is of interest.
- **Local skin energy balance** is an exciting new parameter for different research fields: e.g. sports, nutrition & food supplements, textiles, micro circulation, sleep medicine, special cooling products.

Advantages of Open Chamber Measurement

- Measurement of the TEWL **without any influences** of the probe on the micro climate of the skin (pressure, occlusion, temperature).
- **No waiting** time between the measurements.
- With the “open chamber” method of the Tewameter® TM Hex even **high water loss** values can be detected **accurately** as no water is collected inside the probe.
- Traceable, **elaborate calibration** of humidity, temperature and TEWL to $g/h/m^2$.
- Worldwide **most used** TEWL measurement method (even approved in **space!***).
- Several hundreds of **studies** performed with the Tewameter® prove this fact.

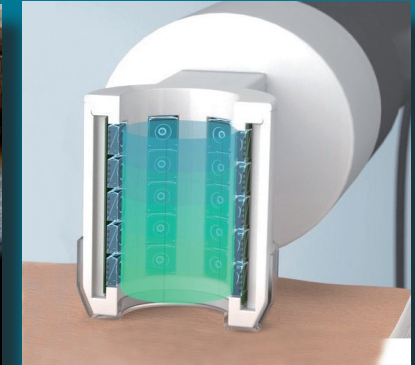

MONADERM

5, rue des Violettes
98000 MONACO
☎ : +377 93 25 26 08
contact@monaderm.com



* Study by DermaTronnier, instruments verified for space by Kayser-Threde GmbH on behalf of the DLR space travel management.



Advantages of Tewameter® TM Hex

- Extremely **accurate, quick and robust** measurement of the TEWL with the information of **30 sensor pairs**.
- A **very stable** measurement is achieved quickly within **20 seconds**.
- Continuous measurements** over longer periods are also possible depending on the application.
- Due to the **high amount of measurement data**, the probe can „see“ the values **like a camera**.
- Unobstructed view** to the measurement surface and **unobstructed evaporation flow**.
- Robust sensor placement** in the wall inside the measurement head.
- Due to the high amount of collected data, measurements not only inside the probe but also on top and below the probe (**ambience and skin surface**).

- Check calibration** with its subsequent **zero offset** can be performed on a daily basis and will compensate “aging effects” to ensure the **high precision over time**.
- First probe with documented, extremely **low measurement uncertainty** visible for each single measurement value.
- Perfect placing on the skin** is possible. The arrow on the probe head shows the direction of diffusion. A message in the software appears if the probe is put on upside down.
- Disposable **hygienic rings**.
- Available for the C+K **MPA-systems** to be operated with the convenient software MPA CTplus.

New Parameters beyond TEWL

- Local Skin Energy Balance:** Skin is constantly emitting energy (heat) in two ways: through **diffusion of warmed air** molecules on top of the skin and through **evaporation cooling**. For the first time, these two can be recorded **separately** during a TEWL measurement. The measured values are expressed in W/m^2 .
- Water vapour concentration CH_2O Skin & Ambience:** This parameter expresses the **absolute humidity** in g/m^3 . The difference between the value measured on the skin and in the ambience is the **actual drive** of the TEWL. In addition, this parameter gives more details about the **measurement conditions** (e.g. atmospheric turbulences).
- In addition, also **temperature & relative humidity (RH)** of the **skin surface and in the ambience** on top of the probe are measured.

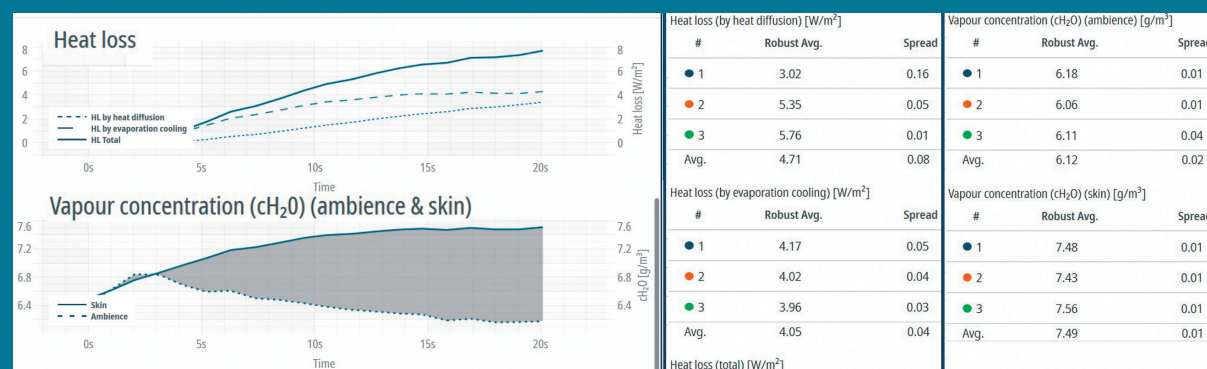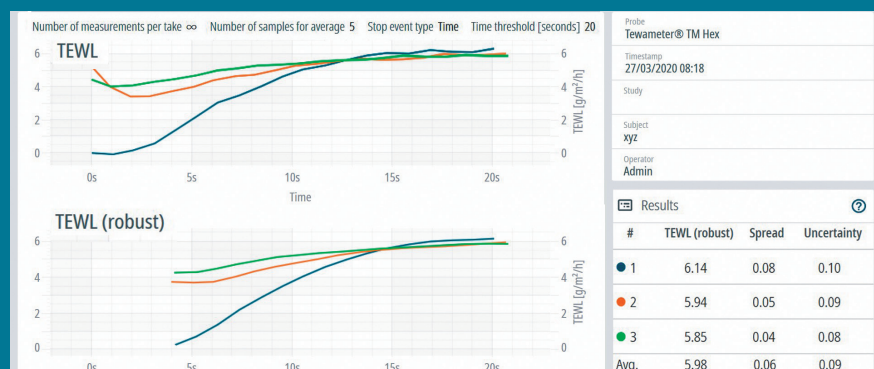

Technical Data

Dim.: Measuring Chamber: Height: 2 cm, \varnothing 1 cm, Probe: Length: 17 cm, Cable length: 1.3 m, Weight: 75 g (incl. cable),
 Measurement principle: “open chamber” measurement of evaporation gradient by 30 sensor pairs inside for temperature & RH;
 Measurement repeatability (confidence interval 99 %): TEWL: $\pm (0.15 \text{ g/h/m}^2 + 1.0 \%)$;
 Measurement uncertainty (max.): TEWL: $\pm (0.5 \text{ g/h/m}^2 + 5.0 \%)$; Operating conditions: T: 10-40° C, RH: 30-70 % RH
Not available as a wireless probe. In this case you need a probe with **Tewameter® TM 300** technology.
 The technical data are preliminary and changes may be made without prior notice.

MONADERM

5, rue des Violettes
 98000 MONACO
 ☎ : +377 93 25 26 08
 contact@monaderm.com

